

alegra

Instructions for Use



CE
0297

PEOPLE HAVE PRIORITY



Turbine handpieces with LED

TE-97 LQ / TE-98 LQ

Roto Quick coupling with generator

RQ-53 / RQ-54

Turbine handpieces without light

TE-95 BC / TE-95 RM

TE-97 / TE-97 BC / TE-97 RM

TE-98 / TE-98 BC / TE-98 RM

Contents

Symbols	4
1. Introduction	6
2. Safety notes	10
3. Product description	14
Roto Quick coupling with generator	14
Turbine TE-97 LQ / TE-98 LQ	15
Turbine TE-97 / TE-98.....	16
Turbine TE-95 BC / TE-97 BC / TE-98 BC.....	17
Turbine TE-95 RM / TE-97 RM / TE-98 RM.....	18
4. Operation	19
Assembly/Removal Roto Quick coupling	19
Assembly/Removal Turbine	23
To change rotary instrument	25
Test run.....	26
5. Hygiene and maintenance	27
General notes	27
Limitations on processing.....	29
Initial treatment at the point of use.....	30
Manual cleaning.....	31

Automated cleaning and lubrication	34
Manual disinfection	35
Automated cleaning and disinfection	36
Drying	37
Inspection, Maintenance and Testing	38
Turbine packaging	43
Sterilization	44
Storage.....	46
6. Maintenance	47
Replacing the rotor.....	47
Cleaning/Replacing the water filter	49
Replacing the generator	51
Replacing the O-rings	53
7. Troubleshooting	54
8. Servicing	56
9. W&H Accessories and spare parts.....	57
10. Technical data	60
11. Disposal.....	65
Explanation of warranty terms.....	66
Authorized W&H service partner	67



WARNING!
(risk of injury)



ATTENTION!
(to prevent
damage occurring)













General explanations,
without risk to
persons or objects



Do not dispose of with
domestic waste

Symbols

packaging / Roto Quick coupling/on the medical device

	CE marking with identification number of the Notified Body		DataMatrix Code for product information including UDI (Unique Device Identification)		Data structure in accordance with Health Industry Bar Code
	Catalogue number		Thermo washer disinfectable		Sterilizable up to the stated temperature
	Serial number		UL Component Recognition Mark indicates compliance with Canadian and U.S. requirements		
	Date of manufacture		Caution! According to Federal law, this medical device may only be sold by or on the order of a dentist, physician or any other medical practitioner licensed by the law of the State in which he or she practices and who intends to use or order the use of this medical device.		

1. Introduction

Customer satisfaction has absolute priority in the W&H quality policy. This medical device has been developed, manufactured and subjected to final inspection according to legal regulations, quality and industry standards.

For your safety and the safety of your patients

Prior to initial use please read the Instructions for use. These explain how to use your medical device and guarantee a smooth and efficient operation.



Observe the safety notes..

Intended use

The dental turbine handpiece is intended for the following applications: Removal of decayed materials, cavities and crown preparation, removal of fillings, finishing of tooth and restoration surfaces.

The Roto Quick coupling is intended for the following applications: Connector for media transfer (air, water, electricity and light) between the supply hose and the dental unit and air driven motors.



Misuse may damage the medical device and hence cause risks and hazards for patient, user and third parties.

Qualifications of the user

We have based our development and design of the medical device on the dentists, dental hygienists, dental employees (prophylaxis) and dental assistants target group

Production according to EU Directive



0297

The medical device meets the requirements of Directive 93/42/EEC.

Responsibility of the manufacturer

The manufacturer can only accept responsibility for the safety, reliability and performance of the medical device when it is used in compliance with the following directions:

- > The medical device must be used in accordance with these Instructions for use.
- > Only the components approved by the manufacturer may be replaced (rotor, O-rings, generator and water filter)
- > Correct the malfunction as described in the instruction for use
- > If it proves impossible to correct the malfunction, please contact an authorized W&H service partner (see page 67).

Skilled application

The medical device is intended only for skilled application according to the intended use as well as in compliance with the valid health and safety at work regulations, the valid accident prevention regulations and in compliance with these Instructions for use.

The medical device should be prepared for use and maintained by staff who have been trained in procedures for infection control, personal safety and patient safety.

Improper use, (e.g., through poor hygiene and maintenance), non-compliance with our instructions or the use of accessories and spare parts which are not approved by W&H, invalidates all claims under warranty and any other claims.

2. Safety notes



- > The operation of the medical device is permitted only on supply units which correspond to the standards IEC 60601-1 (EN 60601-1) and IEC 60601-1-2 (EN 60601-1-2).
- > Before using the medical device for the first time, store it at room temperature for 24 hours.
- > Use only the supply hoses as specified by EN ISO 9168
- > Always ensure the correct operating conditions and cooling function.
- > Always ensure that sufficient and adequate cooling is delivered and ensure adequate suction.
- > In case of coolant supply failure, the medical device must be stopped immediately.
- > Use only the filtered, oil-free and cooled air supplied by dental compressors for drive air
- > Check the medical device for damage and loose parts before each use (e.g. push-button).
- > Do not operate the medical device if it is damaged.



- > Perform a test run before each use.
- > Avoid overheating at the treatment site.
- > Do not use the medical device if there are soft tissue wounds in the mouth. The air pressure can cause septic substances to enter the tissue or trigger embolisms.
- > Do not lift the cheek or tongue with the medical device. Risk of burning due to the push-button heating up!
- > Run the rinse function for the dental unit once per day.
- > Do not use the medical device as a light probe.
- > Do not look directly into the LED.



TE-97 LQ, TE-98 LQ, RQ-53 and RQ-54 are not approved for operation in potentially explosive atmospheres.



Risks due to electromagnetic fields

TE-97 LQ, TE-98 LQ, RQ-53 and RQ-54

The functionality of implantable systems, such as cardiac pacemakers and ICD (implantable cardioverter defibrillator) can be affected by electric, magnetic and electromagnetic fields.

- > Find out if patient and user have implanted systems before using the medical device and consider the application.
- > Weigh the risks and benefits.
- > Keep the medical device away from implanted systems.
- > Make appropriate emergency provisions and take immediate action on any signs of ill-health.
- > Symptoms such as raised heartbeat, irregular pulse and dizziness can be signs of a problem with a cardiac pacemaker or ICD (implantable cardioverter defibrillator).

Hygiene and maintenance prior to initial use




- > The medical device is sealed in PE film and not sterilized when delivered
- > The PE film and the packaging are non-sterilizable



- > Clean, disinfect and lubricate the medical device.
- > Sterilize the turbine and the nozzle cleaner.

3. Product description

Roto Quick coupling with generator

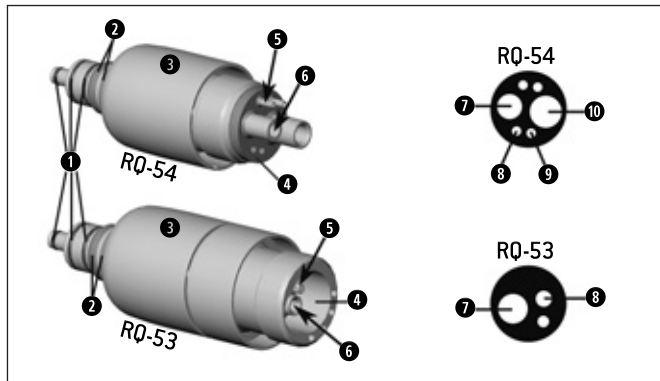


RQ-53 / RQ-54

- ① O-rings
- ② Electrical contacts
- ③ Nut
- ④ Gasket
- ⑤ Water filter with resuction stop
- ⑥ Generator

Connections


- ⑦ Drive air
- ⑧ Water
- ⑨ Spray air
- ⑩ Exhaust

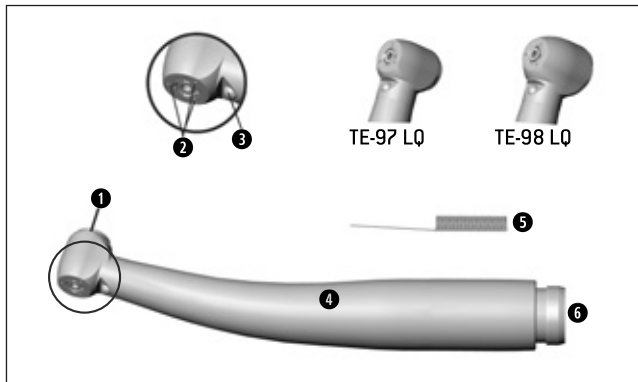

- 1 Push-button
- 2 Spray nozzles
- 3 LED
- 4 Sheath
- 5 Nozzle cleaner
- 6 Roto Quick connection




The turbine handpiece TE-97 LQ / TE-98 LQ may only be used with the Roto Quick coupling RQ-53 / RQ-54.

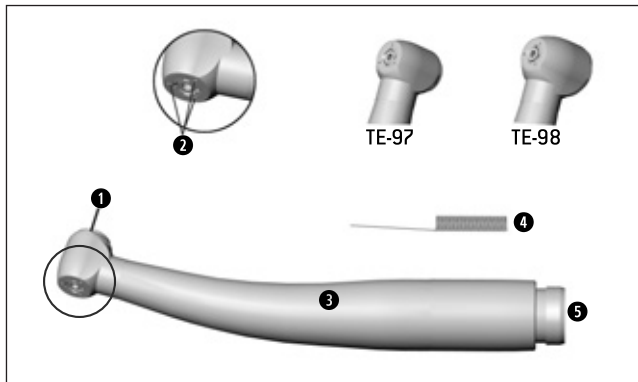

- ① Push-button
- ② Spray nozzles
- ③ Sheath
- ④ Nozzle cleaner
- ⑤ Roto Quick connection

Product description

Turbine TE-95 BC / TE-97 BC / TE-98 BC

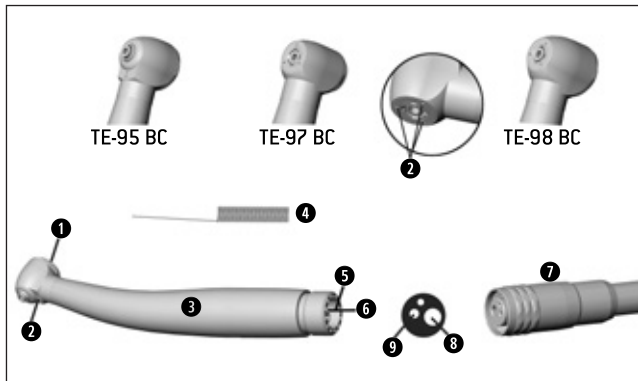


- 1 Push-button
- 2 Spray nozzles
- 3 Sheath
- 4 Nozzle cleaner
- 5 Gasket
- 6 Water filter with resuction stop
- 7 Supply hose

Connections

- 8 Drive air
- 9 Water

Product description

Turbine TE-95 RM / TE-97 RM / TE-98 RM

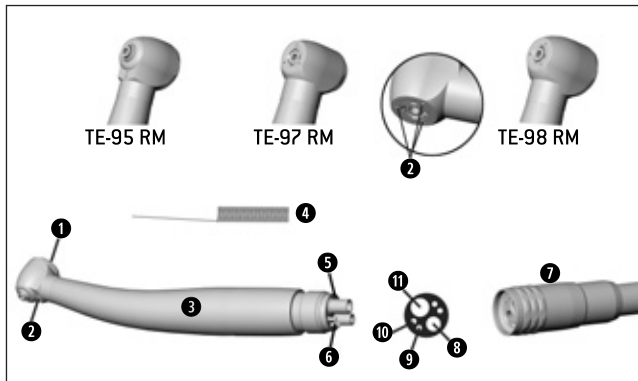


- ① Push-button
- ② Spray nozzles
- ③ Sheath
- ④ Nozzle cleaner
- ⑤ Gasket
- ⑥ Water filter with resuction stop
- ⑦ Supply hose

Anschlüsse

- ⑧ Drive air
- ⑨ Water
- ⑩ Spray air
- ⑪ Exhaust

4. Operation

Assembly/Removal Roto Quick coupling

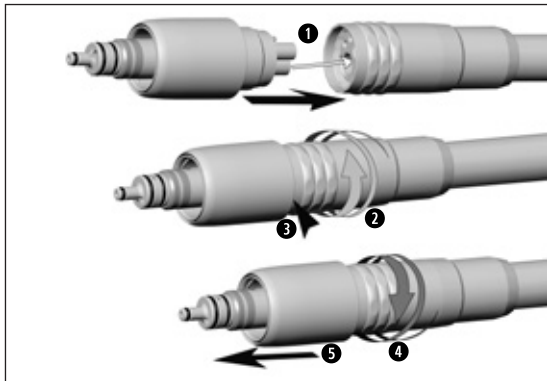

RQ-53 / RQ-54

- 1 Insert the Roto Quick coupling into the apertures of the supply hose.
- 2 Screw the union nut on.



- 3 Check the leak tightness (see page 20) between the Roto Quick coupling and supply hose.

or


- 4 Unscrew the union nut.
- 5 Remove the Roto Quick coupling from the supply hose.

Check leak tightness between Roto Quick coupling and supply hose

- > Block the water outlet at the tip of the Roto Quick coupling with a piece of rubber or leather.
- > Switch on the water.



No water should leak out between the Roto Quick coupling and the supply hose after 10 seconds of blockage.

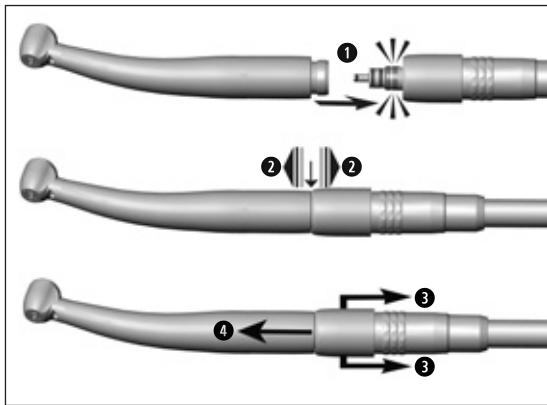

TE-97 LQ / TE-98 LQ / TE-97 / TE-98



Do not assemble or remove the medical device during the operation!

1 Push the turbine handpiece onto the Roto Quick coupling.




2 Verify full engagement.

or

3 Pull the retention sleeve of the Roto Quickcoupling back.

4 Remove the turbine handpiece by pulling in an axial direction.

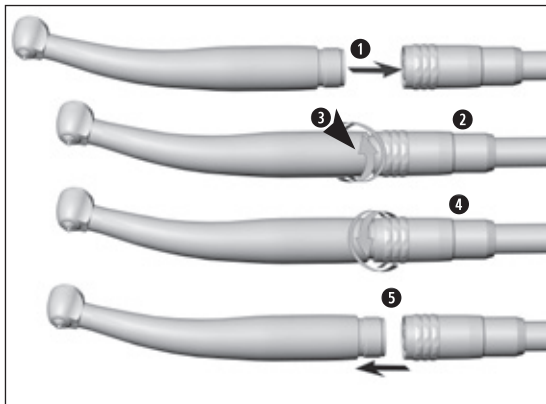

TE-95 BC / TE-97 BC / TE-98 BC


⚠ Do not assemble or remove the medical device during operation!

- ① Insert the turbine handpiece into the apertures of the supply hose.
- ② Screw the union nut on.

⚠ ③ Verify full engagement.
Check the leak tightness

or

- ④ Unscrew on the union nut.
- ⑤ Remove the turbine handpiece from the supply hose.

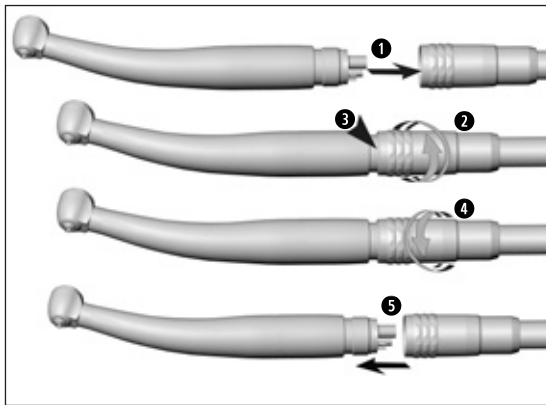

TE-95 RM / TE-97 RM / TE-98 RM

⚠ Do not assemble or remove the medical device during operation!

- ① Insert the turbine handpiece into the apertures of the supply hose.
- ② Screw the union nut on.

**⚠ ③ Verify full engagement.
Check the leak tightness**

or

- ④ Unscrew on the union nut.
- ⑤ Remove the turbine handpiece from the supply hose.

Rotary instruments



- > Use only rotary instruments which are in perfect condition. Follow the operating instructions of the manufacturer
- > Insert the rotary instrument only when medical device is stationary.
- > Do not interfere with the running or slowing down of the rotary instrument.
- > Do not activate the push-button of the medical device during operation or slowing down. This leads to detachment of the rotary instrument resp. heating of the push-button (risk of injury).
- > Only use rotary instruments up to the maximum operating speed stipulated by the manufacturer.



To change rotary instrument

- 1** Insert the rotary instrument.
Activate push-button, at the same time insert the rotary instrument until back stop.



- 2** Verify full engagement.

- 3** Remove the rotary instrument by pushing the push-button.

Test run



Do not hold the medical device at eye level!

- > Insert the rotary instrument.
- > Start the medical device.



In the event of operating malfunctions (e.g., vibrations, unusual noise, overheating, coolant failure or leakage) stop the medical device immediately and contact an authorized W&H service partner.



Follow your local and national laws, directives, standards and guidelines for cleaning, disinfection and sterilization.



> Wear protective clothing, safety glasses, face mask and gloves



> Use only oil-free, filtered compressed air with a maximum operating pressure of 3 bar for manual drying.

Cleaning agents and disinfectants



- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of cleaning agents and/or disinfectants.
- > Use only detergents which are intended for cleaning and/or disinfecting medical devices made of metal and plastic.
- > It is imperative to comply with the concentrations and exposure times specified by the manufacturer of the disinfectant.
- > Use disinfectants which have been tested and found effective by the Verbund für Angewandte Hygiene e.V (VAH = Association for Applied Hygiene), the Österreichischen Gesellschaft für Hygiene, Mikrobiologie und Präventivmedizin (ÖGHMP = Austrian Society for Hygiene, Microbiology and Preventive Medicine), the Food and Drug Administration (FDA) and the U.S. Environmental Protection Agency (EPA).



The user is responsible for validating its process if the specified cleaning agents and disinfectants are not available.



The product lifetime and the medical device's ability to operate correctly are mainly determined by mechanical stress during use and chemical influences due to processing.

- > Send worn or damaged medical devices and/or medical devices with material changes to an authorized W&H service partner.

Processing cycles



- > We recommend a regular service for the W&H medical device after 1,000 processing cycles or one year.



Clean and disinfect the medical device immediately after every treatment, to flush out liquid (e.g., blood, saliva etc.) and to prevent settling on the internal parts.

- > Operate the medical device for at least 10 seconds at idle speed.
- > Ensure that all outlets are rinsed out.



- > Wipe the entire surface of the medical device with disinfectant.
- > Remove the rotary instrument.
- > Remove the turbine from the supply hose.




Note that the disinfectant used during pre-treatment is only for personal protection and cannot replace the disinfectant step after cleaning.

Manual cleaning



Do not place the medical device in liquid disinfectant or in an ultrasonic bath!

- > Clean the medical device under running tap water (<35°C / 95°F).
- > Rinse and brush off all internal and external surfaces.
- > Move moving parts back and forth several times.
- > Remove any liquid residues using compressed air.

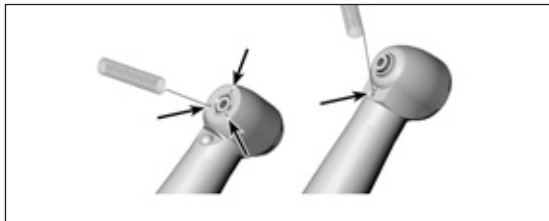


Cleaning of the spray nozzles

- > Clean coolant outlets carefully with the nozzle cleaner to remove dirt and deposits



The nozzle cleaner can be cleaned in an ultrasonic bath and/or in the washer-disinfector

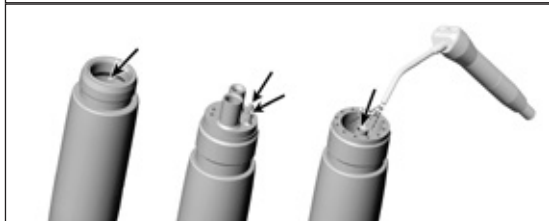


Cleaning of the coolant tubes

- > Blow through the coolant tube using compressed air.



In case of blocked coolant outlets or coolant tubes contact an authorized W&H service partner.

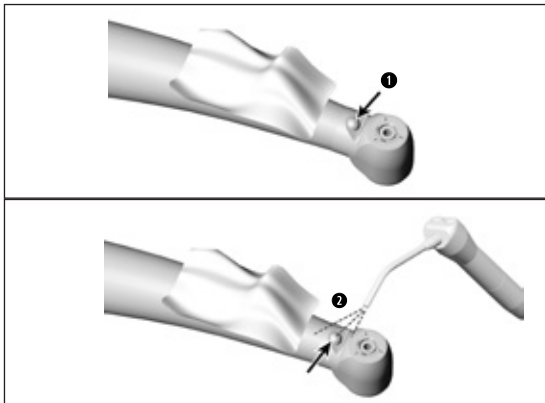

TE-97 LQ / TE-98 LQ Cleaning of the optic outlet



Avoid scratching of the optic outlet!

- 1 Wash the optic outlet with cleaning fluid and a soft cloth.
- 2 Blow the optic outlet dry using compressed air or dry it with a soft cloth.



- > Carry out a visual inspection after each cleaning process.
- > Do not use the medical device if the optic outlet is damaged and contact an authorized W&H service partner.



W&H recommends automated cleaning and lubrication with W&H Assistina 3x3.

> Follow the instructions in the Assistina Instructions for use.



> W&H recommends wiping down with disinfectant.



Evidence of the medical device's basic suitability for effective manual disinfection was provided by an independent test laboratory using the »mikrozid[®] AF wipes« disinfectant (Schülke & Mayr GmbH, Norderstedt).



W&H recommends automated cleaning and disinfection using a washer-disinfector (WD).

- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of washer-disinfectors, cleaning agents and/or disinfectants.



Evidence of the medical device's basic suitability for effective automated disinfection was provided by an independent test laboratory using the >Belimes WD 100< (Firma Belimed AG) washer-disinfector and the >deconex 24 LIQ< cleaning agent (Fa. Borer Chemie) and neutralizer >deconex 26 plus< (Fa. Bohrer Chemie).

- > Cleaning at 65°C (149°F) – 5 minutes
- > Disinfection at 90°C (194°F) – 5 minutes



- > The Roto Quick couplings type RQ-53 / RQ-54 are not approved for cleaning and disinfection using a washer-disinfector.




- > Ensure that the medical device is completely dry internally and externally after cleaning and disinfection.
- > Remove any liquid residues using compressed air.

Inspection



- > Check the medical device after cleaning and disinfection for damage, visible residual soiling and surface changes.
- > Reprocess any medical devices that are still soiled.
- > Sterilize the turbine following cleaning, disinfection and lubrication.

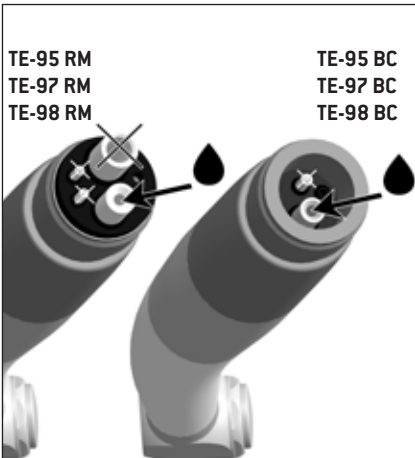

Turbine lubrication



- > Lubricate the dry medical device immediately after cleaning and/or disinfection.
- > Direct the medical device downwards.

Recommended lubrication cycles

- > Essential after every internal cleaning
 - > Before each sterilization
- or
- > After 30 minutes of use or at least once daily
 - > Chucking system once a week

With W&H Service Oil F1, MD-400

- > Follow the instructions on the oil spray can and on the packaging.
- or

With W&H Assistina

- > Follow the instructions in the Assistina Instructions for use.



Lubrication of the chucking system


With W&H Service Oil F1, MD-400

- > Fit the spray adaptor REF 02036100 onto the spray can.
- > Hold the medical device firmly.
- > Press the tip of the spray adaptor firmly into the chucking system
- > Spray for approx. 1 second.

or


With W&H Assistina TWIN / Assistina 301 plus

- > Follow the instructions in the Assistina Instructions for use.

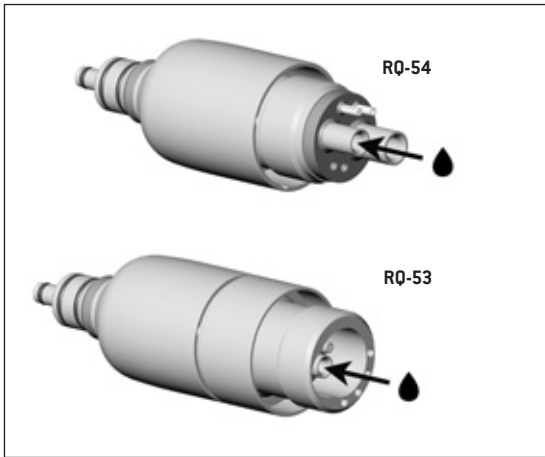

Lubrication of the generator (coupling)

Recommended lubrication cycles

 > 1x a month

see chapter »Maintenance«

With W&H Service Oil F1, MD-400

> Follow the instructions on the oil spray can and on the packaging.

or

With W&H Assistina

> Follow the instructions in the Assistina Instructions for use.

Testing after lubrication



- > Direct the medical device downwards.
- > Operate the medical device so that excess oil can escape.
- > Remove excess oil.



Pack the medical device and the accessories in sterilization packages that meet the following requirements:

- > The sterilization package must meet the applicable standards in respect of quality and use and must be suitable for the sterilization method.
- > The sterilization package must be large enough for the sterilization goods.
- > The filled sterilization package must not be under tension..



W&H recommends sterilization according to EN 13060, EN 285 oder ANSI/AAMI ST79.



- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of steam sterilizers.
- > The program selected must be suitable for the medical device.



- > The Roto Quick couplings type RQ-53 / RQ-54 are not approved for sterilization

Recommended sterilization procedures

- > Fractionated pre-vacuum process (type B)
- > Gravity displacement process (type N)
- > Sterilization time at least 30 minutes at 121°C (250°F) or at least 3 minutes at 134°C (273°F)
- > Maximum sterilization temperature 135°C (275°F)



Evidence of the medical device's basic suitability for effective sterilization was provided by an independent test laboratory using the LISA 522* steam sterilizer (Firma W&H Sterilization S.r.l., Brusaporto (BG)) and the Siroclav S3** gravitation sterilizer (Sirona).

- > Fractionated pre-vacuum process (type B): temperature 134°C (273°F) – 3 minutes*
- > Gravity displacement process (type N): temperature 121°C (250°F) – 30 minutes**


* according to EN 13060, EN 285, ISO 17665 / ** according to ANSI/AAMI ST55 , ANSI/AAMI ST79




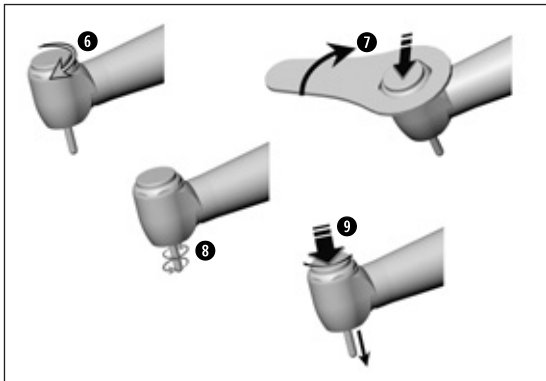
- > Store sterile goods dust-free and dry.
- > The shelf life of the sterile goods depends on the storage conditions and type of packaging.



- > The Roto Quick coupling may be stored on the supply hose.

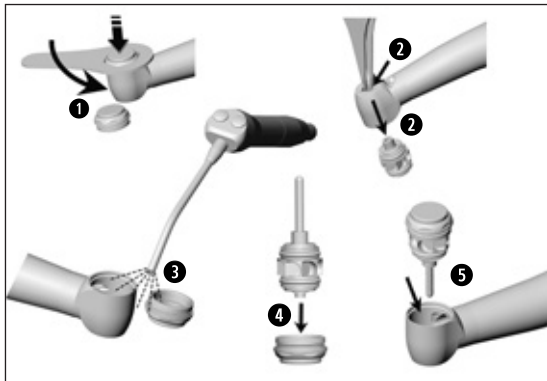


- 1 Unscrew the push-button using the hexagon wrench.
 - 2 Push the rotor out of the turbine head using the tip of a pair of tweezers.
-  Clean the inside of the turbine head and the push-button with a cloth soaked in isopropyl alcohol.
- 3 Blow dry the push-button and the turbine head with compressed air
 - 4 Place the new rotor into the push-button.
 - 5 Place the rotor with the push-button into the turbine head.



- ⑥ Screw the push-button onto the turbine head.
- ⑦ Tighten the push-button using the hexagon wrench.
- ⑧ Check free running of the rotor.
- ⑨ Activate the push-button and remove the mandrel.



- > Perform a test run.
- > Repeat the complete hygiene and maintenance process.

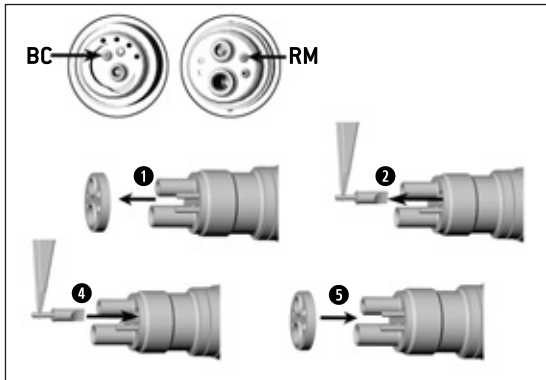

Cleaning/Replacing the water filter


RQ-53 / RQ-54

TE-95 BC / RM, TE-97 BC / RM, TE-98 BC / RM

- 1 Remove the gasket.
- 2 Pull the water filter out using a pair of tweezers.
- 3 Clean the water filter

or

- 4 Insert a new water filter
- 5 Slide on the gasket.

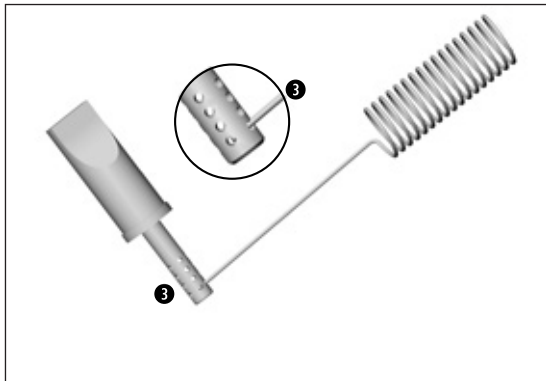

Cleaning the water filter

- 3 Clean outlets carefully with the nozzle cleaner to remove dirt and deposits.




The water filter can be cleaned in an ultrasonic bath.

Turbine:




- > Perform a test run.
- > Repeat the complete hygiene and maintenance process.

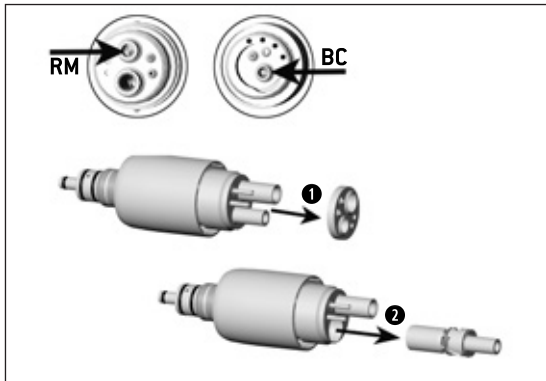


Replacing the generator RQ-53 / RQ-54

- 1 Remove the gasket.
- 2 Pull out the old generator.

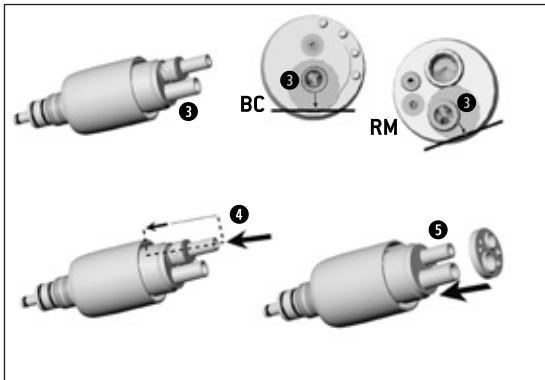

- 3 Position the new generator with the mark aligned with the notch on the Roto Quick coupling.
- 4 Insert the new generator until back stop.
- 5 Slide on the gasket.

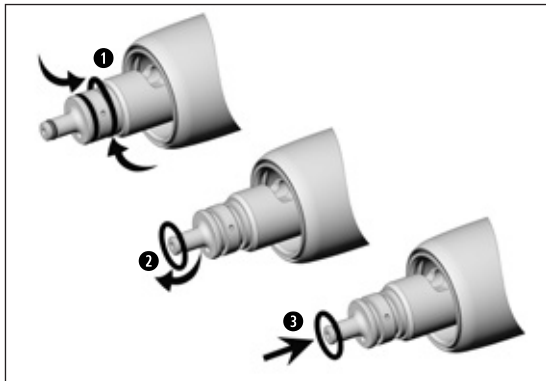

Replacing the O-rings RQ-53 / RQ-54




- > Replace damaged or leaking O-rings immediately.
- > Always replace all the O-rings.
- > Do not use a sharp tool!

- 1 Squeeze the O-ring between your thumb and index finger so that it forms a loop.
- 2 Pull off the O-ring.
- 3 Push the new O-ring on in place.

7. Troubleshooting

Malfunction	Correction of malfunction
Insufficient power	<ul style="list-style-type: none">> Check the connection between the turbine handpiece /Roto Quick coupling and supply hose> Check the operating pressure> Perform an oil service> Check/replace the O-rings> Replace the rotor
Insufficient/no cooling	<ul style="list-style-type: none">> Check the operating pressure> Clean the spray nozzles> Clean/replace the water filter> Check/replace the O-rings

Troubleshooting

Malfunction	Correction of malfunction
Inadequate hold of rotary instrument	<ul style="list-style-type: none">> Perform an oil service> Replace the push-button> Replace the rotor
<p>Insufficient/no light</p>  Attach another LED turbine handpiece to determine whether the LED on the turbine handpiece or the generator in the Roto Quick coupling is defective.	<ul style="list-style-type: none">> Check the operating pressure> Perform an oil service> Lubricate the generator> Replace the generator

8. Servicing

Repairs and returns

In the event of operating malfunctions immediately contact an authorized W&H service partner.

Repairs must only be undertaken by an authorized W&H service partner.



> Ensure that the medical device has been completely processed before returning it.

9. W&H Accessories and spare parts



Use only original W&H accessories and spare parts or accessories approved by W&H.

Suppliers: W&H partners

REF	Description	RQ-53	RQ-54
02015100	Nozzle cleaner	x	x
07508900	O-ring set (2x large, 1x small)	x	x
01000700	BC gasket	x	
02207300	RM gasket		x
06840300	Generator	x	
06793000	Generator		x
07092500	Water filter with resuction stop	x	
07095500	Water filter with resuction stop		x

REF	Description	301	3x2	3x3
000301xx	Assistina 3011 plus	x		
19922000	Assistina 3x2 (MB-200)		x	
19923000	Assistina 3x3 (MB-300)			x
02083500	Adaptor for RQ-53 / TE-95 BC / TE-97 BC / TE-98 BC		x	x
02685000	Base adaptor for RQ-54 / TE-95 RM / TE-97 RM / TE-98 RM	x		
02690400	Adaptor for TE-97 LQ / TE-98 LQ / TE-97 / TE-98		x	
02693000	Adaptor for chucking system	x		
07014500	Adaptor for TE-95 BC / TE-97 BC / TE-98 BC	x		

W&H Accessories and spare parts

REF	Description	TE-97	TE-97 LQ	TE-98	TE-98 LQ
10940021	Service Oil F1, MD-400 (6 pcs)	x	x	x	x
02015100	Nozzle cleaner	x	x	x	x
02229200	Spray cap with nozzle	x	x	x	x
06641900	Push-button			x	x
07548000	Push-button	x	x		
06787500	Rotor with hexagon wrench			x	x
07234100	Rotor with hexagon wrench	x	x		
07508800	Torque wrench	x	x	x	x

W&H Accessories and spare parts

REF	Bezeichnung	TE-95 BC	TE-97 BC	TE-98 BC	TE-95 RM	TE-97 RM	TE-98 RM
10940021	Service Oil F1, MD-400 (6 pcs)	x	x	x	x	x	x
02015100	Nozzle cleaner	x	x	x	x	x	x
02036100	Spray cap with nozzle	x	x	x	x	x	x
06641900	Push-button	x		x	x		x
07548000	Push-button		x			x	
01000700	BC gasket	x	x	x			
02207300	RM gasket				x	x	x
06787500	Rotor with hexagon wrench			x			x
07234100	Rotor with hexagon wrench		x			x	
07507300	Rotor with hexagon wrench	x					
07495400	Rotor with hexagon wrench				x		
07508800	Torque wrench	x	x	x	x	x	x
07092500	Water filter with resuction stop	x	x	x			
07095500	Water filter with resuction stop				x	x	x

10. Technical data

Turbine handpiece		TE-98 / TE-98 LQ	TE-97 / TE-97 LQ
Connection		W&H Roto Quick	
Rotary instruments	ISO 1797 (∅ mm)	1.6 – 0.01	
Maximum length approved by W&H **	(mm)	25	21
Minimum chucking length		until back stop	
Maximum operating part diameter	(mm)	2	
Maximum idle mode speed ($\pm 30,000 \text{ min}^{-1}$)	(min^{-1})	330,000	390,000
Coolant volume	ISO 7785-1, ISO 14457 (ml/min)	> 50	
Water setting range (Recommended water pressure) ***	(bar)	0.7 – 2 (1.5)	
Chip air setting range (Recommended chip air pressure)	(bar)	1.5 – 3 (2)	
Exhaust pressure	(bar)	< 0.5	
Recommended operating pressure	(bar)	2.2 – 2.8	
Air consumption	(l/min)	30 – 45	

min^{-1} (Revolutions per minute)

* see page 63

Technical data

Turbine handpiece		TE-95 BC / TE-98 BC	TE-97 BC
Connection according to standard	EN ISO 9168:2009	Type 1: Borden 2-hole	
Rotary instruments	ISO 1797 (∅ mm)	1.6 – 0.01	
Maximum length approved by W&H **	(mm)	25	21
Minimum chucking length		until back stop	
Maximum operating part diameter	(mm)	2	
Maximum idle mode speed ($\pm 30,000 \text{ min}^{-1}$)	(min^{-1})	330,000	390,000
Coolant volume	ISO 7785-1, ISO 14457 (ml/min)	> 50	
Water setting range (Recommended water pressure) ***	(bar)	0.7 – 2 (1.5)	
Chip air setting range (Recommended chip air pressure)	(bar)	1.5 – 3 (2)	
Exhaust pressure	(bar)	< 0.5	
Recommended operating pressure	(bar)	2.2 – 2.8	
Air consumption	(l/min)	30 – 45	

min^{-1} (Revolutions per minute)

* see page 63

Technical data

Turbine handpiece		TE-95 RM / TE-98 RM	TE-97 RM
Connection according to standard	EN ISO 9168:2009	Type 3: Standard 4-hole	
Rotary instruments	ISO 1797 (∅ mm)	1.6 – 0.01	
Maximum length approved by W&H**	(mm)	25	21
Minimum chucking length		until back stop	
Maximum operating part diameter	(mm)	2	
Maximum idle mode speed ($\pm 30,000 \text{ min}^{-1}$)	(min^{-1})	330,000	390,000
Coolant volume	ISO 7785-1, ISO 14457 (ml/min)	> 50	
Water setting range (Recommended water pressure) ***	(bar)	0.7 – 2 (1.5)	
Chip air setting range (Recommended chip air pressure)	(bar)	1.5 – 3 (2)	
Exhaust pressure	(bar)	< 0.5	
Recommended operating pressure	(bar)	2.2 – 2.8	
Air consumption	(l/min)	30 – 45	

min^{-1} (Revolutions per minute)

* see page 63

Technical data

Roto Quick coupling	RQ-53	RQ-54
Connection according to standard	EN ISO 9168:2009	Type 1: Borden 2-hole Type 3: Standard 4-hole
Recommended operating pressure	(bar)	2.2 – 2.8



Power and speed data of turbine handpieces are largely dependent on the quality of the turbine hoses used and may therefore differ from the specified values



** When using longer rotary instruments the user must ensure by correct selection of the operating conditions, that there is no danger to the user, patient or third parties.

***Chip air pressure / water pressure must be set at the same time
The chip air pressure must be higher than the water pressure

Temperature information



Temperature of the medical device on the operator side: maximum 55°C (131°F)

Temperature of the medical device on the patient side: maximum 50°C (122°F)

Temperature of the working part (rotary instrument): maximum 41°C (105.8°F)

Ambient conditions

Temperature during storage and transport

-40°C to +70°C (-40°F to +158°F)

Humidity during storage and transport

8 % to 80 % (relative), non-condensing

Temperature during operation

+10°C to +35°C (+50°F to +95°F)

Humidity during operation:

15 % to 80 % (relative), non-condensing

11. Disposal



Ensure that the parts are not contaminated on disposal.



Follow your local and national laws, directives, standards and guidelines for disposal.

- > Medical device
- > Waste electrical equipment
- > Accessories, consumables, spare parts
- > Packaging

Explanation of warranty terms

This medical device has been manufactured with great care by highly qualified specialists. A wide variety of tests and controls guarantee faultless operation. Please note that claims under warranty can only be validated when all the directions in the Instructions for use have been followed.

As manufacturer, W&H is liable for material or manufacturing defects within a warranty period of 12 months from the date of purchase.

We accept no responsibility for damage caused by incorrect handling or by repairs carried out by third parties not authorized to do so by W&H!

Claims under warranty accompanied by proof of purchase, must be sent to the vendor or to an authorized W&H service partner. The provision of service under warranty extends neither the warranty period nor any other guarantee period.

12 months warranty

Authorized W&H service partner

Find you nearest W&H service partner at <http://wh.com>

Simply go to the menu option »Service« for full details. Alternatively please contact:

W&H (UK) Limited, Unit 6, Stroud Wood Business Centre, Park Street, St Albans, AL2 2NJ Hertfordshire
t + 44 1727874990, f + 44 1727872254, E-Mail: technical.uk@wh.com

W&H IMPEX INC., 6490 Hawthorne Drive, Windsor, Ontario, N8T 1J9, Canada
t + 1 519 9446739, f + 1 519 9746121, E-Mail: service.ca@wh.com

W&H IMPEX INC., 33091 W Jefferson Ave., Brownstown, MI-48173, USA
t + 1 800 265 6277, +1 519 944 6739, f +1 519 974 6121, E-Mail: service.us@wh.com

W&H Austria GmbH, Ignaz-Glaser-Straße 53, 5111 Bürmoos, Austria
t +43 6274 6236-239, f +43 6274 6236-890, E-Mail: office.at@wh.com

A-DEC AUSTRALIA CO. INC., Unit 8, 5-9 Ricketty Street, Mascot NWS 2020, Australia
t + 61 2 83324000, f + 61 2 83324099, E-Mail: a-dec@a-dec.com.auw

Manufacturer

W&H Dentalwerk Bürmoos GmbH
Ignaz-Glaser-Straße 53, 5111 Bürmoos, Austria

t +43 6274 6236-0,
office@wh.com

f +43 6274 6236-55
wh.com

Form-Nr. 50817 AEN
Rev. 002 / 08.04.2019
Subject to alterations